




Drying

Drying is the separation of excess solvent from product. This common method is used for stabilisation of substances, reduction of quantity, sample dosage, analysis or change of physical and chemical characteristics.

Theoretical background

The drying process involves the separation of liquid from material by volatilisation or evaporation. Evaporation occurs if the vapour pressure of the liquid is greater than that of atmospheric pressure. Thermal drying process consists of three sub-processes: the heat transfer from the atmosphere to the damp material, phase conversion of the solvent (from liquid to gas) and evacuation of the solvent vapour. Energy required for the drying

process is conducted from the surface of the sample into the centre using thermal conduction. This heat conductivity depends on the humidity content of the sample, the less moisture content, the less conductivity. Hence, drying processes can lead to thermal decomposition, therefore protocols and methodology have been developed to ensure product quality.

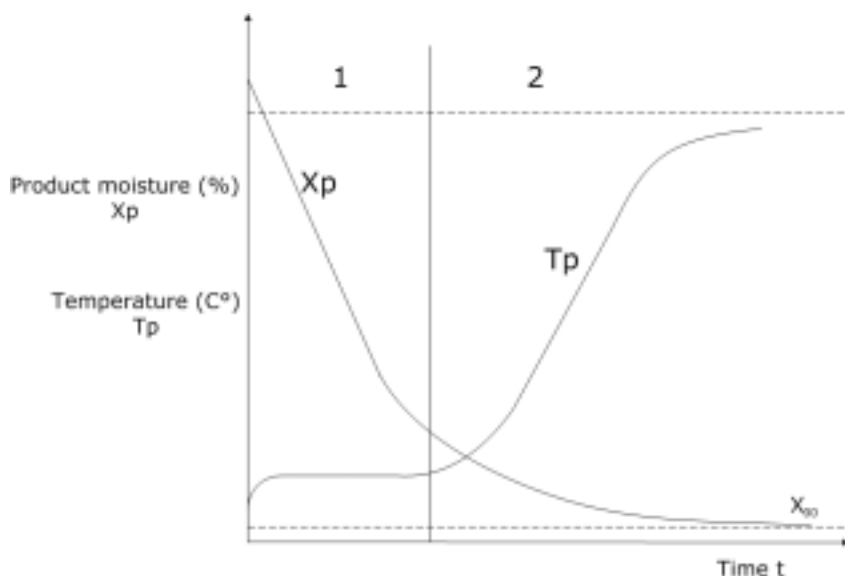

The diagram above shows that moisture content decreases significantly over time, t , until it reaches an equilibrium value. The temperature of substance T_p increases until it reaches the value of

drying temperature. In the 1st drying section the temperature of the material is almost constant and moisture content of the material decreases linearly with the time.



Method


The BÜCHI Glass Oven B-585 is the perfect product for drying small quantities, as it heats the sample indirectly, via radiation. The glass oven essentially consists of two glass tubes, one placed inside the other. Heating takes place through a completely transparent, electrically conductive semiconductor layer on the inner tube, whereby the resistance under voltage, produces heat.

The second, outer glass tube prevents the damage of heat tube and at the same time protects against direct contact with the charged part.

The operating angle can be adjusted from 0° to 90° using a lever. This flexibility of being able to tilt the oven chamber increases the quality and speed of the drying process.

Drying accessory

The drying accessory consists of three parts. The drying tube (1) in which material can be placed directly or in a container. This tube is inserted into the oven for the drying process. To improve the drying process, a drying agent (3) may be placed in the drying hood (2), to absorb the evaporated moisture. The stopcock (4) is used for the evacuation and aeration of the sample chamber. Because the oven utilises radiant heat, heat transfer to the sample is fast and efficient.

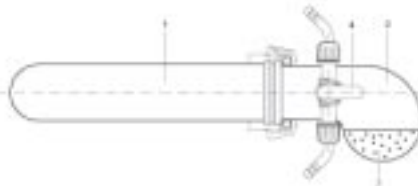

The drying process can be performed in two ways:

Large quantity of the material can be filled directly into the drying tube or in a sample container placed inside the drying tube itself, providing it can withstand the temperature.

This type of drying is normally avoided in hygroscopic samples, because it can absorb moisture whilst being transferred to another container.



The second method, the material is filled placed in the intended storage container before drying and this is placed in the drying tube.

The drying oven is then operated in vertical position. The advantages of this method is that it avoids the need to transfer the sample into another container and that the sample container may be closed immediately.



Drying of solid substances with rotation

While drying, some substances form solid layer on their surface, which substantially extends the drying time. This can be prevented by rotation preferably in a drying flask with grooves. The flask can be rotated using the electrical ball tube drive, glass frit is melted in the corresponding vapour duct in order to prevent material loss by drying with rotation.



Quality in your hands

BÜCHI Labortechnik AG
Postfach
9230 Flawil
Schweiz
Tel. +41 71 394 63 63
Fax +41 71 394 65 65
buchi@buchi.com
www.buchi.com

BUCHI Analytical Inc.
19 Lukens Drive
New Castle
Delaware 19720
USA
Tel. +1 302 652 3000
Fax +1 302 652 8777
us-sales@buchi.com
www.buchi-analytical.com

BÜCHI Labortechnik GmbH
Postfach 10 03 51
45003 Essen
Deutschland
Freecall 0800 414 0414
Fax +49 201 237 082
deutschland@buchi.com
www.buechigmbh.de

BUCHI Analytical Ltd.
Link House
Stakehill Industrial Park
Middleton
Manchester M24 2RH
Great Britain
Tel. +44 161 654 60 60
Fax +44 161 643 75 10
uk-sales@buchi.com
www.buchi-analytical.co.uk

BÜCHI Labortechnik GmbH
Branch Office Netherlands
Postbus 142
3340 AC Hendrik Ido Ambacht
The Netherlands
Tel. +31 78 684 94 29
Fax +31 78 684 94 30
netherlands@buchi.com
www.buchi.com

Nihon **BUCHI** K.K.
7F Kojima Bldg. 2-11-10 Ueno
Taito-ku
Tokyo 110-0005
Japan
Tel. +81 3 5807 5599
Fax +81 3 5807 5598
nihon@buchi.com
www.buchi.com

BÜCHI Italia s.r.l.
Centro Direzionale, Milano Fiori
Pal. A-4, Strada 4
20090 Assago (MI)
Italia
Tel. +39 02 824 50 11
Fax +39 02 57 51 28 55
italia@buchi.com
www.buchi.it

BUCHI Sarl
5, rue du Pont des Halles
Z.A. du Delta
94656 Rungis Cedex
France
Tél. +33 1 56 70 62 50
Fax +33 1 46 86 00 31
france@buchi.com
www.buchi.fr

BACC BUCHI
ASEAN Competence Center
c/o Becthai Bangkok
300 Phaholyothin Road
Samsennai, Phayathai
Bangkok 10400
Thailand
Tel. +66 1 829 49 10
bacc@buchi.com
www.buchi.com

BUCHI SMP Services Private Ltd.
201, Magnum Opus
Shantinagar Industrial Area
Vakola, Santacruz (East)
Mumbai 400 055
India
Tel. +91 22 569 89 450
Fax +91 22 569 89 452
smplisp@vsnl.com
www.buchi.com